WONDERLAND LABS

Certificate of Analysis

08 APRIL 2026

CRYO / MIT



CLIENT:	**ZMB ENTERPRISES**	**SAMPLE SET:**	**178090**
Sample Type:	Liquid	Date Acquired:	04/08/2026
Sample Weight:	2mL	Acquisition Method:	MIT-EVO_R2026-01
Dilution:	0.1	Testing ID:	GRD-MIT_160266.D
Vial:	Vial 32	Date Processed:	04/08/2026
Injection Volume:	5.0 µl	Run Time:	27 min
Prepped By:	Sarah T.	Calibration ID:	20260105

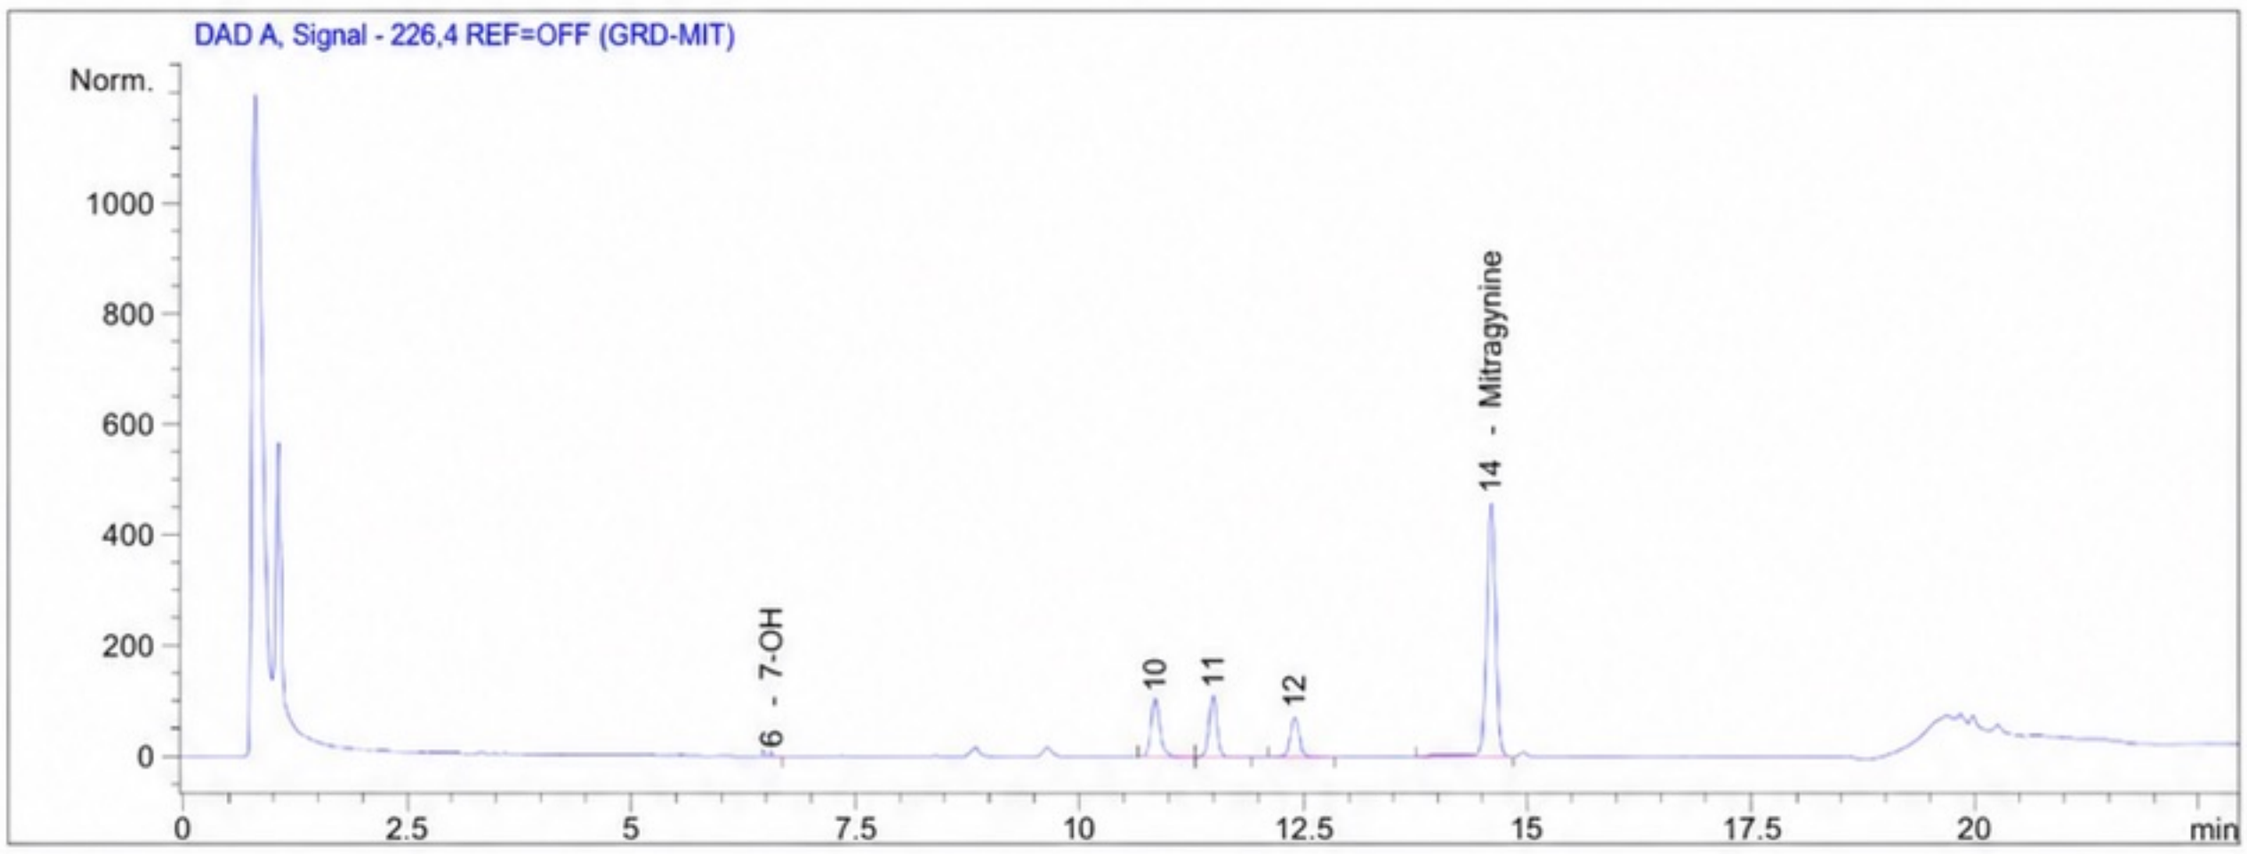

#	Analyte	RT (min)	Area (mAU*s)	Amt (µg/mL)	Alkaloid	Total %
1	Mitragynine	14	6358	298	$C_{23}H_{30}N_2O_4$	**2.98**
2	7-Hydroxymitragynine	6	N/D	N/D	$C_{23}H_{30}N_2O_5$	N/D
3	Paynantheine	10	1367	67	$C_{23}H_{28}N_2O_4$	0.67
4	Speciogynine	11	1484	72	$C_{23}H_{30}N_2O_4$	0.72
5	Speciociliatine	12	934	46	$C_{23}H_{30}N_2O_4$	0.46
6						

Mitragynine Content: **30** mg/mL (THREE ZERO)

Adulterants (Y/N): None Detected

Identity Confirmed: YES

SEAL OF AUTHENTICITY

VERIFIED BY:

Quality Assurance:

Wonderland Labs | 1341 Distribution Way, Ste 16, Vista CA 92081 | www.Wonderland-Labs.com | Info@Wonderland-Labs.com | (800) 647-3154